

Total Prostate Specific Antigen (PSA) ELISA

REF CAN-TPSA-4300

RUO

Effective Date: June 24, 2024

Version: RUO-12.0

1. INTENDED PURPOSE & USE

For the quantitative measurement of Total Prostate Specific Antigen (PSA) in human serum by an ELISA (Enzyme-Linked Immunosorbent Assay).

For Research Use Only. Not for use in diagnostic procedures.

2. LIMITATIONS RELATED TO INTENDED PURPOSE & USE

- This kit is intended for research use only and is not to be used for any diagnostic procedures.

3. PRINCIPLE OF THE TEST

The Total PSA ELISA is a two-step capture or 'sandwich' type immunoassay. The assay makes use of two highly specific monoclonal antibodies: A monoclonal antibody specific for Total PSA is immobilized onto the microplate and another monoclonal antibody specific for a different epitope of PSA is conjugated to horse radish peroxidase (HRP conjugate). In the first incubation step, PSA present in the specimen samples, calibrators and controls is bound by the antibody immobilized onto the microplate. Excess and unbound materials are removed by a washing step.

In the second incubation step, HRP conjugate antibody (HRP conjugate) is added, which binds specifically to any immobilized PSA, thus forming a sandwich complex. Unbound HRP conjugate is removed by a washing step. Next, the TMB substrate (enzyme substrate) is added which reacts with HRP to form a blue coloured product that is directly proportional to the amount of PSA present. The enzymatic reaction is terminated by the addition of the stopping solution, converting the colour from blue to yellow. The absorbance is measured on a microplate reader at 450 nm. A set of calibrators is used to plot a calibrator curve from which the amount of Total PSA in specimen samples and controls can be directly read.

4. PROCEDURAL CAUTIONS AND WARNINGS

- This kit is for use by trained laboratory personnel (professional use only). For laboratory *in vitro* use only.
- Practice good laboratory practices when handling kit reagents and specimens. This includes:
 - Do not pipette by mouth.
 - Do not smoke, drink, or eat in areas where specimens or kit reagents are handled.
 - Wear protective clothing and disposable gloves.
 - Wash hands thoroughly after performing the test.
 - Avoid contact with eyes; use safety glasses; in case of contact with eyes, flush eyes with water immediately and contact a doctor.
- Users should have a thorough understanding of this protocol for the successful use of this kit. Reliable performance will only be attained by strict and careful adherence to the instructions provided.
- Do not use the kit beyond the expiry date stated on the label.
- If the kit reagents are visibly damaged, do not use the test kit.
- Do not use kit components from different kit lots within a test and do not use any component beyond the expiration date printed on the label.

- All kit reagents and specimens must be brought to room temperature and mixed gently but thoroughly before use. Avoid repeated freezing and thawing of specimens.
- When the use of water is specified for dilution or reconstitution, use deionized or distilled water.
- Immediately after use, each individual component of the kit must be returned to the recommended storage temperature stated on the label.
- A calibrator curve must be established for every run.
- It is recommended to all customers to prepare their own control materials or serum pools which should be included in every run at a high and low level for assessing the reliability of results.
- The controls (included in kit) must be included in every run and their results must fall within the ranges stated in the quality control certificate; a failed control result might indicate improper procedural techniques or pipetting, incomplete washing, or improper reagent storage.
- When dispensing the substrate and stopping solutions, do not use pipettes in which these liquids will come into contact with any metal parts.
- The TMB Substrate is sensitive to light and should remain colourless if properly stored. Instability or contamination may be indicated by the development of a blue colour, in which case it should not be used.
- Do not use grossly hemolyzed, grossly lipemic, icteric or improperly stored serum.
- Samples or controls containing azide or thimerosal are not compatible with this kit, they may lead to false results.
- Samples values above the measuring range of the kit may be reported as >100 ng/mL. If further dilution and retesting is required, only calibrator A may be used to dilute serum samples. The use of any other reagent may lead to false results.
- Avoid microbial contamination of reagents.
- To prevent the contamination of reagents, use a new disposable pipette tip for dispensing each reagent, sample, calibrator, and control.
- To prevent the contamination of reagents, do not pour reagents back into the original containers.
- Kit reagents must be regarded as hazardous waste and disposed of according to local and/or national regulations.
- Consumables used with the kit that are potentially biohazardous (e.g., pipette tips, bottles or containers containing human materials) must be handled according to biosafety practices to minimize the risk of infection and disposed of according to local and/or national regulations relating to biohazardous waste.
- This kit contains 1 M sulfuric acid in the stopping solution component. Do not combine acid with waste material containing sodium azide or sodium hypochlorite.
- The use of safety glasses, and disposable plastic, is strongly recommended when manipulating biohazardous or bio-contaminated solutions.
- Proper calibration of the equipment used with the test, such as the pipettes and absorbance microplate reader, is required.
- If a microplate shaker is required for the assay procedure, the type and speed of shaker required is stated in the REAGENTS AND EQUIPMENT NEEDED BUT NOT PROVIDED section. Both the type and speed of shaker used can influence the optical densities and test results. If a different type of shaker and/or speed is used, the user is responsible for validating the performance of the kit.
- Do not reuse the microplate wells, they are for SINGLE USE only.
- To avoid condensation within the microplate wells in humid environments, do not open the pouch containing the microplate until it has reached room temperature.
- When reading the microplate, the presence of bubbles in the wells will affect the optical densities (ODs). Carefully remove any bubbles before performing the reading step.

5. SAFETY CAUTIONS AND WARNINGS

5.1 BIOHAZARDS

The reagents should be considered a potential biohazard and handled with the same precautions applied to blood specimens. All human specimens should be considered a potential biohazard and handled as if capable of transmitting infections and in accordance with good laboratory practices.

The calibrators and controls provided with the kit contain material(s) of human origin that have been tested and found to be negative for the presence of Hepatitis B, Hepatitis C and HIV 1 & 2. However, no test method can offer complete assurance that any viable pathogens are absent. Therefore, these components should be considered a potential biohazard and handled with the same precautions as applied to any blood specimen, following good laboratory practices.

5.2 CHEMICAL HAZARDS

Avoid direct contact with any of the kit reagents. Specifically avoid contact with the TMB Substrate (contains tetramethylbenzidine) and Stopping Solution (contains sulfuric acid). If contacted with any of these reagents, wash with plenty of water and refer to SDS for additional information.

6. SPECIMEN COLLECTION, STORAGE AND PRE-TREATMENT

6.1 Specimen Collection & Storage

Approximately 0.1 mL of serum is required per duplicate determination. Collect 4–5 mL of venous blood into an appropriately labelled tube and allow it to clot. Centrifuge at room temperature and carefully transfer the serum into a new storage tube or container. Serum samples may be stored at 2–8°C for up to 24 hours or at -10°C or lower if the analyses are to be done at a later date. at -10°C or lower for up to 1 month.

6.2 Specimen Pre-Treatment

Specimen pre-treatment is not required.

7. REAGENTS AND EQUIPMENT NEEDED BUT NOT PROVIDED

- Calibrated single-channel pipette to dispense 25 µL.
- Calibrated multi-channel pipettes to dispense 50 µL and 100 µL.
- Calibrated multi-channel pipettes to dispense 300 µL (if washing manually).
- Automatic microplate washer (recommended).
- Microplate shaker:
 - Orbital shaker (3 mm diameter) set to 600 rpm or
 - Reciprocating shaker (1.5" stroke length) set to 180 oscillations/minute.
- Disposable pipette tips.
- Distilled or deionized water.
- Calibrated absorbance microplate reader with a 450 nm filter and an upper OD limit of 3.0 or greater.

8. REAGENTS PROVIDED

1. **MPL** Microplate

Contents:	One anti-PSA monoclonal antibody-coated 96-well (12x8) microplate in a resealable pouch with desiccant.
Format:	Ready to Use
Storage:	2–8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for four weeks.

2. **HRP CONJ CONC** HRP Conjugate Concentrate

Contents:	One bottle containing anti-PSA monoclonal antibody-Horse Radish Peroxidase (HRP) conjugate in a protein-based buffer with a non-mercury preservative.		
Format:	Concentrated; Requires Preparation		
Volume:	0.3 mL/bottle		
Storage:	2–8°C		
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for four weeks.		
Preparation of HRP Conjugate Working Solution:	<table border="1" style="margin-left: 20px;"> <tr> <td>X51</td> <td>Dilute 1:51 Before Use</td> </tr> </table> Dilute 1:51 in assay buffer before use (e.g., 40 µL of HRP conjugate concentrate in 2 mL of assay buffer). If the whole plate is to be used dilute 240 µL of HRP conjugate concentrate in 12 mL of assay buffer. Discard any that is left over.	X51	Dilute 1:51 Before Use
X51	Dilute 1:51 Before Use		

3. **CAL A – F** Calibrator A – F

Contents:	Six bottles of calibrator containing specified PSA concentrations. Protein-based buffer with a non-mercury preservative. Prepared by spiking buffer with defined quantities of PSA.
	Listed below are approximate concentrations, please refer to vial labels for exact concentrations. Concentrations: 0, 0.5, 2, 10, 40, 100 ng/mL.
Format:	Ready to Use
Volume:	Calibrator A: 2.0 mL/bottle Calibrator B-F: 0.5 mL/bottle
Storage:	2–8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for four weeks.

4. **CONTROL 1 – 2** Control 1 – 2

Contents:	Two bottles of control containing different PSA concentrations. Protein-based buffer with a non-mercury preservative. Prepared by spiking buffer with defined quantities of PSA. Refer to the QC certificate for the target values and acceptable ranges.
Format:	Ready to Use
Volume:	0.5 mL/bottle
Storage:	2–8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for four weeks.

5. **ASY** **BUFF** **Assay Buffer**


Contents:	One bottle containing a protein-based buffer with a non-mercury preservative.
Format:	Ready to Use
Volume:	30 mL/bottle
Storage:	2–8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for four weeks.

6. **TMB** **SUB** **TMB Substrate**

Contents:	One bottle containing tetramethylbenzidine and hydrogen peroxide in a non-DMF or DMSO containing buffer.
Format:	Ready to Use
Volume:	16 mL/bottle
Storage:	2–8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for four weeks.

7. **STOP** **Stopping Solution**

Contents:	One bottle containing 1M sulfuric acid.
Format:	Ready to Use
Volume:	6 mL/bottle
Storage:	2–8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for four weeks.
Safety:	Refer to product SDS.

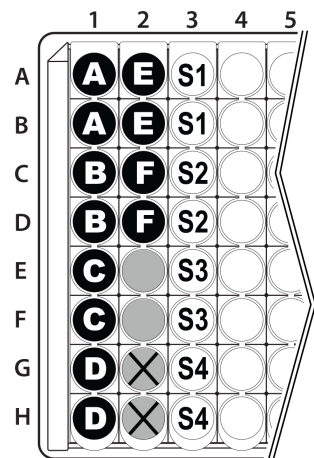


Warning





8. **WASH** **BUFF** **CONC** **Wash Buffer Concentrate**

Contents:	One bottle containing buffer with a non-ionic detergent and a non-mercury preservative.
Format:	Concentrated; Requires Preparation
Volume:	50 mL/bottle
Storage:	2–8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for four weeks. Following Preparation: The wash buffer working solution is stable for 2 weeks following preparation, assuming Good Laboratory Practices are adhered to. To prevent microbial growth, prepare the wash buffer working solution in a clean container and store under refrigerated conditions (2-8°C) when not in use.
Preparation of Wash Buffer Working Solution:	<div style="border: 1px solid black; padding: 2px; display: inline-block;">X10</div> Dilute 1:10 Before Use Dilute 1:10 in distilled or deionized water before use. If the whole microplate is to be used dilute 50 mL of the wash buffer concentrate in 450 mL of distilled or deionized water.

9. RECOMMENDED ASSAY LAYOUT



Legend

-  Calibrators
-  Control 1
-  Control 2
-  Samples

10. ASSAY PROCEDURE

Specimen Pre-Treatment: None
All kit components, controls and specimen samples must reach room temperature prior to use. Calibrators, controls, and specimen samples should be assayed in duplicate. Once the procedure has been started, all steps should be completed without interruption.
<ol style="list-style-type: none"> After all kit components have reached room temperature, mix gently by inversion. Prepare the HRP Conjugate Working Solution and Wash Buffer Working Solution (See section 8. <i>Reagents Provided</i> section, 2. <i>HRP Conjugate Concentrate</i> and 8. <i>Wash Buffer Concentrate</i>). Plan the microplate wells to be used for calibrators, controls, and samples. See section 9. <i>Recommended Assay Layout</i>. Remove the strips from the microplate frame that will not be used and place them in the bag with desiccant. Reseal the bag with the unused strips and return it to the refrigerator. Pipette 25 µL of each calibrator, control, and specimen sample into assigned wells. Pipette 100 µL of the Assay Buffer into each well (the use of a multi-channel pipette is recommended). Incubate the microplate on a microplate shaker** for 60 minutes at room temperature. Wash the microplate wells with an automatic microplate washer (preferred) or manually as stated below. <i>Automatic:</i> Using an automatic microplate washer, perform a 3-cycle wash using 300 µL/well of Wash Buffer Working Solution (3 x 300 µL). One cycle consists of aspirating all wells then filling each well with 300 µL of Wash Buffer Working Solution. After the final wash cycle, aspirate all wells and then tap the microplate firmly against absorbent paper to remove any residual liquid. <i>Manually:</i> For manual washing, perform a 3-cycle wash using 300 µL/well of Wash Buffer Working Solution (3 x 300 µL). One cycle consists of aspirating all wells by briskly emptying the contents of the wells over a waste container, then pipetting 350 µL of Wash Buffer Working Solution into each well using a multi-channel pipette. After the final wash cycle, aspirate all wells by briskly emptying the contents over a waste container and then tap the microplate firmly against absorbent paper to remove any residual liquid. Pipette 100 µL of the HRP Conjugate Working Solution into each well (the use of a multi-channel pipette is recommended). Incubate the microplate on a microplate shaker** for 30 minutes at room temperature. Wash the microplate wells again as stated in step 7. Pipette 100 µL of TMB Substrate into each well (the use of a multi-channel pipette is recommended). Incubate the microplate on a microplate shaker** for 10-15 minutes at room temperature. Pipette 50 µL of Stopping Solution into each well (the use of a multi-channel pipette is recommended) in the same order and speed as was used for addition of the TMB Substrate. Gently tap the microplate frame to mix the contents of the wells. Measure the optical density (absorbance) in the microplate wells using an absorbance microplate reader set to 450 nm, within 20 minutes after addition of the Stopping Solution. ** See section 7. <i>Reagents And Equipment Needed But Not Provided</i> for microplate shaker options.

11. CALCULATIONS

- Calculate the mean optical density for each calibrator, control and specimen sample duplicate.
- Use a 4-parameter or 5-parameter curve fit with immunoassay software to generate a calibrator curve.
- The immunoassay software will calculate the concentrations of the controls and specimen samples using the mean optical density values and the calibrator curve.
- If a sample reads more than 100 ng/mL and needs to be diluted and retested, then dilute with calibrator A not more than 1:8. The result obtained must be multiplied by the dilution factor.

12. QUALITY CONTROL

When assessing the validity of the test results, the following criteria should be evaluated:

- The values obtained for the kit controls are within the acceptable ranges as stated in the QC certificate.
- The results of any external controls that were used meet the acceptable ranges.

13. TYPICAL DATA

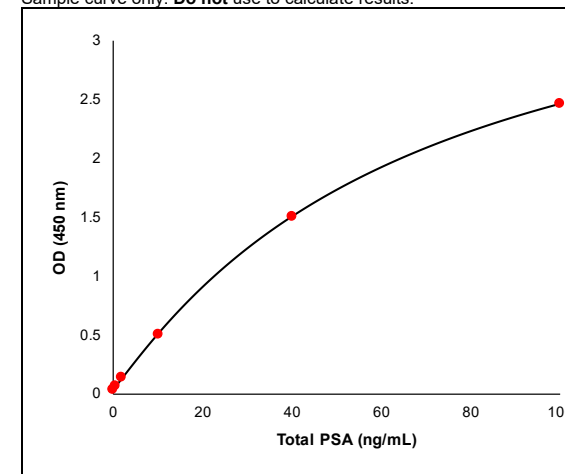
13.1 TYPICAL TABULATED DATA

Sample data only. **Do not** use to calculate results.





















Calibrator	Mean OD (450 nm)	% Binding	Value (ng/mL)
A	0.045	2	0
B	0.067	3	0.5
C	0.145	6	2
D	0.513	21	10
E	1.51	61	40
F	2.464	100	100
Unknown	0.208	-	3.3

13.2 TYPICAL CALIBRATOR CURVE

Sample curve only. **Do not** use to calculate results.



14. SYMBOLS GLOSSARY

Symbol	Definition	Symbol	Definition
	Catalogue number		Manufacturer
	Batch code		Date of manufacture
	In vitro diagnostic medical device		Biological risks
	Unique Device Identifier		Consult instructions for use
	Dilute 1:# Before Use		Prescription only: Device restricted to use by or on the order of a physician
	Quantity		Keep away from sunlight
	Use-by date		Authorized representative in the European Community/ European Union
	Do not re-use		Temperature limit
	Caution		Contains sufficient for <n> tests
	Lyophilized		For Research Use Only. Not for use in diagnostic procedures.
The definitions of symbols used for kit component names are described in the <i>Reagents Provided</i> section.			

15. CHANGE HISTORY

Previous Version:	11.0 (Combined)	New Version:	RUO-12.0
Changes:	<p>New IFU format with numbered headings.</p> <p>HEADING Removal of country-specific regulatory information. Addition of RUO symbol. Removed all performance characteristics, reference ranges and literature/references.</p> <p>1. INTENDED PURPOSE & USE Addition: For Research Use Only. Not for use in diagnostic procedures.</p> <p>2. LIMITATIONS RELATED TO INTENDED PURPOSE & USE All limitations removed and replaced with: This kit is intended for research use only and is not to be used for any diagnostic procedures.</p> <p>4. PROCEDURAL CAUTIONS AND WARNINGS Additional cautions and warnings added. Some previous limitations added to this section.</p> <p>7. REAGENTS AND EQUIPMENT NEEDED BUT NOT PROVIDED Addition of microplate shaker options.</p>		

8. REAGENTS PROVIDED

Addition of symbols for all components and safety information if applicable.
In-use stability statement added for all components.
Control low and high now called control 1 and 2, respectively.

9. RECOMMENDED ASSAY LAYOUT

New section added.

10. ASSAY PROCEDURE

Component names revised to match symbol definitions.

11. CALCULATIONS

Removed instructions for manually plotting calibrator curve.

12. QUALITY CONTROL

New section added.

13.1 TYPICAL TABULATED DATA

Table data updated.

13.2 TYPICAL CALIBRATOR CURVE

Curve updated based on updated table data.

14. SYMBOLS GLOSSARY

Addition of symbols and definitions.

15. CHANGE HISTORY

New section added.

16. GENERAL INFORMATION

Addition of product complaints, warranty and limitation of liability sections.
Removal of EC REP information.

Build: v1.4D

BASE: v12.0

16. GENERAL INFORMATION



Diagnostics Biochem Canada (DBC) Inc.
384 Neptune Crescent
London, Ontario, Canada N6M 1A1
Tel: (519) 681-8731
Fax: (519) 681-8734
e-mail: dbc@dbc-labs.com
www.dbc-labs.com

Product Complaints

In the case of product complaints, the user shall submit in writing to the distributor or manufacturer a description of the complaint and provide accompanying data and/or information.

Warranty

DBC guarantees that the product is free of defects and will perform within the product specifications when the product is used prior to the expiration date, according to the intended purpose and use, and according to the instructions for use provided with the product. Any deviations from the intended purpose and use, instructions for use, modifications to kit components or use beyond the expiration date will invalidate any warranty claims.

Limitation of Liability

DBC liability in all circumstances whether in tort (including negligence) or at common law, and for any damage or loss, including but not limited to loss of profit and loss of sales, suffered whether direct, indirect, consequential, incidental or special is limited to the purchase price of the product(s) in question.